Troubleshooting.

If problem cannot be corrected, consult your Dealer/Home Care equipment provider.

PROBLEM	PROBABLE CAUSE	REMEDY
A. No flow	1. Cylinder valve closed	1. Turn on cylinder
	2. Conserver in "OFF"	2. Set to prescribed position setting
	3. Cylinder empty	3. Replace cylinder
	4. Dial not at setting	 Set dial so indicator points to a setting
	5. Conserver not sensing breath	5. Check position of cannula in nose Do not breathe through mouth
B. Leaking at Cylinder Connection	 Missing or defective O-ring Seal 	1. Replace O-ring Seal




Refer to User Manual for complete operating instructions, warnings and cautions.

Precision Medical. Inc.

300 Held Drive • Northampton, PA 18067 800-272-7285 • 610-262-6090 • fax: 610-262-6080

504808 12/05 Printed in USA

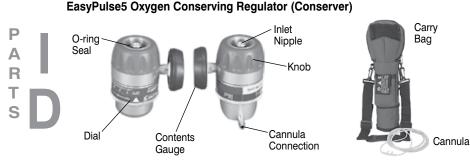

Cylinder Valve

Inspect Conserver and Cylinder Valve for damage or contaminants. Do NOT use if any are found. "Crack" cylinder valve by opening the valve slightly and closing.



S

STEP

Ensure Conserver is in the OFF position and O-ring Seal is in place. Align Nipple with recessed hole in the cylinder. Hand tighten Knob. Do NOT use tools.



D

S

S T

E١

Ρ

When using a Precision Medical Carry Bag, slide the cylinder into the bag with the gauge facing the mesh. Attach the cannula to the Conserver's Outlet Connection.



Slowly open the cylinder valve. Turn Dial to the prescribed setting. Zip the bag closed.





Place cannula in nostrils and breathe through nose to begin Oxygen flow. If using a bag adjust the straps for maximum comfort.



When finished using:

